




तुलसीपुर उपमहानगरपालिका



नगर कार्यपालिकाको कार्यालय

प.सं. 208२/08३

च.नं. AD-2५८४

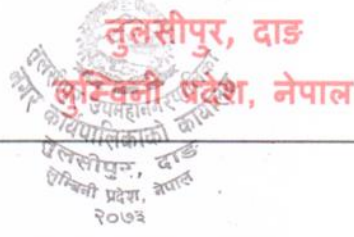

मिति: २०८३/१/१६


बिषय: दररेट उपलब्ध गराउने सम्बन्धमा ।

श्री सूचिकृत सप्लायर्स तथा फर्महरु सबै ।

तुलसीपुर उपमहानगरपालिका नगर कार्यपालिकाको कार्यालयको आ.व. २०८२/०८३ को स्वीकृत बजट तथा कार्यक्रमबाट राप्ती आँखा अस्पताल रक्षाचौर, दाङको लागि Dry Eye Therapy Machine खरिद गर्नुपर्ने भएकाले सो सामग्री खरिदका गर्न लागत अनुमान तयार गर्ने प्रयोजनको लागि यसै पत्रसाथ संलग्न स्पेसिफिकेशन बमोजिमका सामग्रीहरु मु.अ.कर बाहेकको प्रचलित बजार दररेट भन्दा बढी नहुने गरी दररेट उपलब्ध गराइ दिनुहुन अनुरोध छ ।

तपसिल:

- संस्था वा फर्म दर्ताको प्रमाणपत्र,
- स्थायी लेखा नम्बर वा मूल्य अभिवृद्धि कर दर्ताको प्रमाणपत्र,
- कर चुक्ता प्रमाण पत्र,
- आवश्यकता अनुसारको व्यवसायिक इजाजतपत्र ।

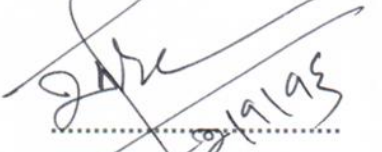
२०८३/१/१६
केश्वरराज पाण्डे
प्रमुख प्रशासकीय अधिकृत

Dry Eye Diagnostic Device

Manufacturer:

Brand:

Type/Model:

Country of Origin/Year:



S.N.	Technical Specifications	Bidder's Compliance Sheet			For Official use only
		Yes	No	Page no	Remarks
1	Examination Performed				
1.1	Dry eye diagnostic device is an instrument used for individual analysis of tear film that allows to carry out quick detailed structural research of the tear composition (i.e. Lipid, Aqueous, Mucin).				
2	System Requirements				
2.1	Dry eye diagnostic instrument, complete unit with all standard accessories.				
3	Descriptions of Functions				
3.1	Should have quantitative measurement of lipid layer thickness.				
3.2	Should measure Tear meniscus height upto 5 mm.				
3.3	Should image the morphology of the meibomian glands with analysis				
3.5	Should have functions for visualization of blepharitis and presence of demodex				
3.6	Should have functions of ocular redness classification, pupillometry and white to white measurement, marginal reflex distance.				
3.7	Should be able to capture high quality anterior segment image				
3.8	Should have doctor patient interaction app which is found in Android				

Handwritten signature/initials

Handwritten signature/initials



S.N.	Technical Specifications	Bidder's Compliance Sheet			For Official use only
3.9	Should be able to capture NIBUT, LLT, TMH in just 15 sec				
3.1	Should have standard treatment suggesting protocol				
4	Technical Data				
4.1	Should have image resolution of at least 5MP				
4.2	Should have multi shot, video acquisition mode				
4.3	Should have both auto focus and manual focus				
4.4	Should have infrared LED – blue, red and white LED light source				
5	Hardware Requirement for Diagnostic Device				
5.1	Should have colored, sensitive to infrared, yellow filtered camera				
5.2	Should have complete PC unit with latest intel Core i7, SSD drive, 8GB RAM, Screen resolution 1600*900 and Genuine Microsoft Windows 8,10 professional (Pro) x64 bit				
5.3	Color printer				
6	Accessories				
6.1	All standard accessories required to operate system should be supplied				
7	Operating Environment				
7.1	The system offered shall be designed to be stored and to operate normally under the conditions of the purchaser's country. The country should include Power supply, Climate, Temperature, Humidity.				
7.2	Power supply : 220 – 240V AC, 50 HZ fitted with appropriate plug. The power cable shall be at least 3m in length.				
8	Documentation/User Training				

2112

(Handwritten signature)



S.N.	Technical Specifications	Bidder's Compliance Sheet			For Official use only
8.1	User manual in English should be provided				
8.2	Must provide user training including how to use and maintain equipment until complete familiarity				
8.3	Should provide at least 3 installations base satisfaction letter				
9	Standard And Safety Requirement				
9.1	Should have CE and USFDA approved certificate				
10	Warranty				
10.1	Comprehensive warranty of 1 year on the system				
10.2	During warranty period supplier must ensure corrective/breakdown maintenance whenever required				
<p>Bidders must fully complete the Technical Specification Form (TSF), clearly indicating compliance or non-compliance, and provide a supporting brochure with highlighted features and page numbers. Failed to do so led to rejection of bids.</p>					

[Handwritten signature]

[Handwritten signature]